

Engineered Science

DOI: https://dx.doi.org/10.30919/es8d796



Numerical Analysis of Specific Absorption Rate and Temperature Distribution in Human Eye due to Moving Electromagnetic Source

Deepshikha Bhargava and Phadungsak Rattanadecho*

Abstract

The study presents a numerical analysis of the absorption of electromagnetic (EM) radiation in human eye as a result of the exposure from moving EM source. A two-dimensional eye model consisting of six types of tissues is exposed to a moving EM source operating at 900 and 1800 MHz frequencies for a time period of 10 minutes. The EM source irradiate the eye and the energy gets absorbed in the eye layers. Electric field intensity, specific absorption rate (SAR), and temperature distribution in the eye for both frequencies are calculated by solving a coupled model of electromagnetic wave and bio-heat transfer module. From the results it is concluded that the EM source's position, and the dielectric and thermal properties of the eye highly influence the absorption of EM radiation in the eye layers. SAR and temperature in the eye do not seem to correlate with each other. The highest value of SAR (31.54 W/kg) and highest value of temperature (37.72 °C) are found in the cornea layer of the eye for 1800 MHz frequency when the EM source is at a minimum distance with the eye. Effect of the size of EM source on the EM absorption in the eye layers has also been investigated. It is observed that larger size of EM source causes higher absorption of EM radiation in the eye layers. The resultant value of SAR in some cases exceeded the limited value of 2W/kg by ICNIRP whereas the temperature increase is found to be below the safety levels.

Keywords: Human eye; Moving electromagnetic source; Specific absorption rate; Temperature; Finite element method.

Received: 06 June 2022; Revised: 12 November 2022; Accepted: 29 November 2022.

Article type: Research article.

1. Introduction

Eyes are the most delicate part of our human body. Due to the absence of the outer skin layer and the lack of blood flow, they are more prone to the outer surroundings. Study of EM wave interaction with the eye tissues has been a topic of interest for years. Temperature increase above some degrees in the eye is capable of causing thermal damage and adverse physiological effects in the tissues. Health organizations such as ICNIRP^[1] and IEEE^[2] have established limited EM exposure for the human body, measured in terms of specific absorption rate (SAR), where the main concern for the adverse effect in the eye has been the temperature increase in it. An increase of 3-4 °C temperature can cause cataract formation in the eye,

Center of Excellence in Electromagnetic Energy Utilization in Engineering (CEEE), Department of Mechanical Engineering, Faculty of Engineering, Thammasat University (Rangsit Campus), 99 moo 18, Klong Luang, Pathum Thani 12120, Thailand.

*E-mail: ratphadu@engr.tu.ac.th (P. Rattanadecho)

where a temperature of 41 °C can cause posterior capsular opacities (PCO). [3-5] Previous studies have shown formation of cataract in rabbit's eye after 2-3 hours of exposure from microwave, whereas no cataract was formed in monkey's eye. [6-8] The study of heat transfer analysis in the human eye as a result of the exposure from EM wave is sparse. Most of the literature only discuses SAR, [9-11] which is obvious considering that the safety guidelines are only based on it. However, in order to study the realistic situation and to get a better understanding of the phenomena, studying heat transfer analysis in the eye as a result of the EM radiation exposure is necessary.

Thermal analysis in the human eye has been discussed previously, Zarei *et. al*^[12] studied the effect of sunglasses, with different ambient conditions, on the heat transfer in the eye and Firoozan *et. al*^[13] studied the effect of different ambient conditions, convection coefficient *etc.* on the temperature increase in the eye to help control the eye temperature during the eye surgeries. Temperature increase due to EM radiation

exposure has also been studied,[14,15] Bernardi et. al[15-17] included temperature distribution along with the SAR in the human body. They found that temperature and SAR in the eve do not correlate with each other and depend on the frequency of the EM source. Lower frequency has higher wavelength which penetrates deeper into the tissue leading to higher temperature. However, For SAR, higher values were found at higher frequencies. Similar observation was made by Flyckt et, al.[18] in their study they found higher value of SAR in the deeper layers of the human eye model for higher frequency. In contrary to Bernardi et. al[15-17] findings, Hirata et. al[19,20] found SAR and temperature increase in the eye for plane and oblique incident waves to be corelating with each other.

Our lab has also been studying the SAR and temperature distribution in the human tissues as an exposure from EM radiation. Wesaapan et. al[5,14,21-23] have extensively studied effect of EM radiation on the SAR and temperature increase in the tissues such as eyes, body, head of adult and child, human genitals etc. Effect of metal objects such as jewelry and spectacles in proximity with the mobile phone radiation on the head and eye tissues has also been studied.[24] It has been concluded that studying temperature distribution along with SAR is important as factors like - type of the radiation source, position of the radiation source from the tissues, and the dielectric and thermal properties of tissues could influence the EM absorption leading to a noncorrelation between SAR and temperature.

In the literature, interaction of EM radiation with the eye has been studied when the EM source is in a stationary position. Meaning, the radiation has been incident on the eye from one direction and one position only. Situation when an EM source is continuously moving in front of the eye irradiating the larger region has not been discussed until now. This could be the case when a person is getting exposed to some sort of moving EM radiation emitting device at places like industries, home etc. Some good example of it can be seen at convenience stores where the employees get exposed to the microwave radiation from the microwave oven several times throughout the day while standing and heating the food for their customers or a person on a video call keeps moving his hand and exposes the eyes to the mobile phone radiation in a continuous varying position, as shown in Fig. 1. Hence, studying a case when the eye gets exposed to a continuous moving EM source is important and could be useful for people who often find themselves in such situations.

Exposing the eye to a continuous moving EM source is somewhat similar to scanning a tissue. Some examples of continuous scanning of tissues can be seen in microwave

emitting sources, like electrodes and antennas, are used to irradiate/scan the tissues at smaller-smaller portions one by one in order to construct an inside image of the tissues. Likewise, in laser therapy, the laser is projected on the skin on a smaller portion one by one. For scanning the eye (exposing it to a continuous moving source) a small EM radiation source needs to be created.

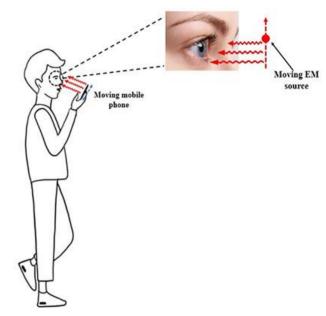


Fig. 1 Human eye exposed to the moving electromagnetic source.

Continuous scanning has been performed by creating a gaussian function and using it as a moving source for scanning the tissue. Kabiri et. al^[27] made a moving laser source using gaussian function and studied the effect of its velocity and intensity on the temperature distribution in the skin and the kidney during the thermotherapy. Ma et. al^[28] irradiated a three-dimensional human tissue with a moving laser and studied the burn damage distribution on it. It was found that the size of the laser source and its speed highly influenced the thermal damage on the skin. Apart from this, pruet et. al^[29] used a moving laser heat source to study its effect on the thermal behavior of the metal during the selective laser melting.

In this study, hence, a small EM radiation source is created with the help of a gaussian function and used to scan the eye. The human eye is modelled in two-dimension consisted of seven types of tissues, shown in Fig. 2. The EM radiation source operating at 900 and 1800 MHz frequencies takes 10 minutes to scan the whole eye area from the left side (Fig. 3). Electric field, SAR and temperature distribution inside the eye as a result of the exposure from moving EM source at both frequencies are calculated. COMSOLTM Multiphysics software based on Finite Element Method (FEM) is used for imaging (MI) and laser therapy. [25,26] In MI system, microwave solving the coupled model of EM wave propagation (TE mode)

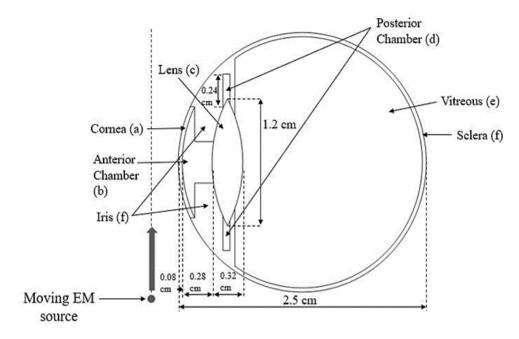


Fig. 2 Physical model of human eye.

and bio-heat transfer analysis. Maxwell's equations are used radiating at 1000W power is considered for this study. The EM to solve the EM wave propagation analysis inside the tissues as well as in its surrounding area.^[14,30] Whereas, classical heat conduction equation is used to solve the heat transfer analysis in the tissues.^[19,31,32] Moreover, the effect of the size of EM radiation source on the SAR and temperature increase in the eye has also been discussed.

2. Problem formulation

2.1 Physical model

EM absorption in a human eye as a result of the exposure from moving EM source is studied (Fig. 1). A two-dimensional eye model is created to study the EM wave and heat transfer analysis in the eye tissues as a result of the exposure from moving EM source, shown in Fig. 2. This eye model has previously been used by Shafahi and Vafai.[33] The eye model consists of seven types of tissues namely posterior chamber, vitreous, sclera, lens, cornea, anterior chamber, and iris. The dielectric and thermal properties of the tissues are taken from Tables 1 and 2, respectively. In this study, sclera and iris are considered as one homogenous tissue, hence, they have the same properties. An EM radiation source of size 5 mm, operating at 900 and 1800 MHz frequencies and at 1000Watt power is created and scanned on the left side of the eye model with the help of gaussian function (Fig. 3). The radiated power is chosen considering an extreme/worst case. Situation when a person may get exposed to poor-quality devices who radiates more power. Continuous exposure of these bad quality devices may cause harmful effect on the eye. Hence, an EM source

source moves over the port boundary (Fig. 3) and scans the whole eye in 10 minutes. EM absorption and temperature in the eye as a result of EM exposure are calculated using COMSOLTM Multiphysics software based on FEM.

Table 1. Dielectric properties of eye tissues at different frequencies.[15,34]

Tissue	Frequency: 900 MHz		Frequency: 1800 MHz	
	$arepsilon_r$	σ (S/m)	$arepsilon_r$	σ (S/m)
Cornea (a)	52.00	1.85	55.0	2.32
Anterior	73.00	1.97	75.0	2.40
Chamber (b)				
Lens (c)	51.30	0.89	41.1	1.29
Posterior	73.00	1.97	75.0	2.40
Chamber (d)				
Vitreous (e)	74.30	1.97	73.7	2.33
Sclera (f)	52.10	1.22	52.7	1.68
Iris (f)	52.10	1.22	52.7	1.68

Table 2. Thermal properties of eye tissues. [35]

	1 1	,	
Tissue	$\rho(\text{kg/m}^3)$	k (W/°C)	$C_p(J/kg^{\circ}C)$
Cornea (a)	1050	0.58	4178
Anterior Chamber (b)	996	0.58	3997
Lens (c)	1000	0.4	3000
Posterior Chamber	996	0.58	3997
(d)			
Vitreous (e)	1100	0.603	4178
Sclera (f)	1050	1.0042	3180
Iris (f)	1050	1.0042	3180

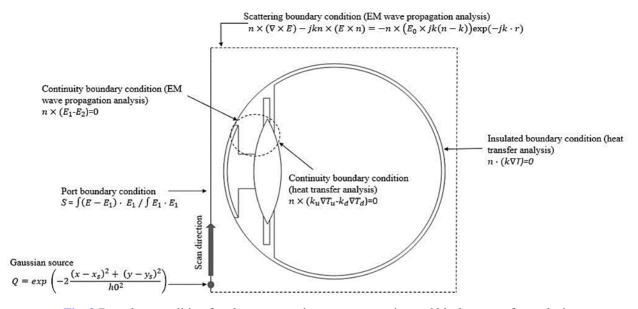


Fig. 3 Boundary condition for electromagnetic wave propagation and bio-heat transfer analysis.

2.2 Equations for Electromagnetic wave propagation EM wave in TE mode at 1000-Watt power. analysis

The EM radiation source moves continuously in the upward direction irradiating the eye. The EM wave propagation, inside the eye tissues and in the surroundings, is numerically solved using Maxwell's equations. In order to reduce the computation time while not compromising with the results, the analysis has been carefully performed in two-dimension. To further simplify the calculation of EM wave propagation analysis, following assumptions are made:[5]

- 1. The EM wave propagate and interacts with the eye tissues in two dimensions.
- 2. The Eye model surroundings are truncated using scattering boundary condition.
- 3. The dielectric properties of the eye tissues are uniform and 2.2.2 moving source constant throughout the calculations.
- 4. The propagation of EM wave is in Transverse Electric mode (TE mode).

The EM wave propagation in the free space and through the eye tissues are solved using Maxwell's equation in TE mode:

$$\nabla \times \left(\frac{1}{\mu_r} \nabla \times E\right) - k_0^2 \left(\varepsilon_r - \frac{j\sigma}{\omega \varepsilon_0}\right) E = 0 \tag{1}$$

where E is Electric field (V/m), μ_r is the relative magnetic permeability, ε_r is the relative dielectric constant, ε_0 = 8.8542×10^{-12} F/m is the permittivity of free space, σ is the electrical conductivity (S/m), and k_0 is the free space wave number (m^{-1}) .

2.2.1 Boundary condition for wave propagation analysis

Port boundary condition is applied on the outer region at the left side of the eye model, as shown in Fig. 3. The port emits

$$S = \frac{\int (E - E_1) \cdot E_1}{\int E_1 \cdot E_1}$$
 (2)

Continuity boundary condition is applied between air and eye model and in between the eye tissues:

$$n \times (H_1 - H_2) = 0 (3)$$

The area outside the eye model is truncated using the scattering boundary condition:

$$n \times (\nabla \times E_z) - jkE_z - jkE_z = -jk(1 - k \cdot n)E_{0z}exp(-jk \cdot r)$$
(4)

where k is the wave number (m^{-1}) , σ is the electric conductivity (S/m), n is normal vector, $j = \sqrt{-1}$, and E_0 is the incident plane wave (V/m).

A gaussian function is created on the port boundary condition acting as an EM radiation source, [29] moving in the upward direction as shown in Fig. 3. The gaussian function takes total 10 minutes to cover the port. The size of the gaussian function with its movement in the upward direction on the port is expressed as Eq. (5).

$$Q = \exp\left(-2\frac{(x-x_s)^2 + (y-y_s)^2}{h0^2}\right)$$
 (5)

where, x_s and y_s are the horizontal and vertical positions of the source in x and y directions, respectively, and ho is the height of the source, The EM source moves only in the y direction, hence the movement in the x position stays the same.

2.3 Interaction of Electromagnetic wave with human tissues

The EM wave propagates in free space, incident on the eye

known as specific absorption rate (SAR). The SAR in the eye tissues are calculated and can be expressed as[5,14] —

$$SAR = \frac{\sigma}{\rho} |E|^2 \tag{6}$$

where E is the electric field intensity (V/m), σ is the electric conductivity (S/m), and ρ is the tissue density.

2.4 Equation for heat transfer analysis

The temperature distribution inside the eye tissues is studied using classical heat conduction equation. The initial temperature of the eye model is set to 37°C. For simplifying the thermal analysis, following assumption are made^[5] -

- 1. The thermal properties of the eye tissues remain constant and uniform.
- 2. The tissues are biomaterial.
- 3. There is no energy exchange, phase change, and chemical reaction occurring in the tissues.

Classical heat conduction equation is used to calculate the temperature distribution in the tissues, shown in Eq. (7).[12] The transient equation is capable of effectively analyzing the heat transfer occurring in the tissues-

$$\rho C \frac{\partial T}{\partial t} = \nabla \cdot (k \nabla T) + Q_{\text{ext}}$$
 (7)

where ρ is the tissue density (kg/m³), C is the heat capacity of tissue (J/kg °C), k is the thermal conductivity of tissue (W/m °C), T is the tissue temperature (°C), and Q_{ext} is the external heat source term (electromagnetic heat-source density) (W/m^3) .

 Q_{ext} is the external heat source term equal to the resistive heat generated by electromagnetic field (electromagnetic power absorbed), defined as:[5]

$$Q_{ext} = \frac{1}{2} \sigma_{tissue} |E|^2 = \frac{\rho}{2} \cdot SAR$$
 (8)

Boundary condition for heat transfer analysis

An insulated boundary condition is applied on the outer surface of the eye model to isolate it from the surroundings as the heat transfer analysis is only considered within the eye-

$$n \cdot (k \nabla T) = 0 \tag{9}$$

Continuity boundary condition is applied between the eye layers showing there is no contact resistance between them-

$$\nabla T_u = \nabla T_d \tag{10}$$

$$n \cdot (k_u \nabla T_u - k_d \nabla T_d) = 0 \tag{11}$$

2.5 Numerical method

Finite element method (FEM) is used to calculate the SAR and 3.1 Numerical validation temperature in the eye tissues as a result of the exposure from moving EM source. The first step of FEM is to divide the obtained temperature distribution in the eye model (without

and gets absorbed by the eye tissues. This absorbed energy is geometry in several small parts of different shapes called meshing, shown in Fig. 4. The coupled model of EM wave and bioheat transfer are then solved numerically. The numerical analysis is performed on each part of the mesh in order to get the precise results. To make sure that the obtained results are independent of the number of mesh elements, a mesh convergence test is performed. Fig. 5 shows the graph between the number of mesh elements and the temperature in the cornea layer of the eye. The analysis is performed for 1800 MHz frequency when the EM source is at 317 sec position. It is observed that after 2865 number of mesh elements the value of temperature becomes consistent. This shows that the obtained results after that certain number is independent of mesh elements. At this point it is fair to assume that the results are reliable and precise.




Fig. 4 Two-dimension mesh model of human eye.

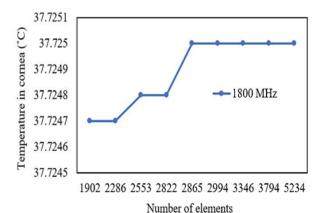


Fig. 5 Grid convergence graph between number of mesh elements and temperature.

3. Results and discussions

The proposed numerical model is verified by comparing the

the electromagnetic module) with the results of Shafahi and Vafai. [33] It is to be noted that the comparison has been made for the static EM source, since it is really difficult to find a similar case in the literature. The heat transfer coefficient and ambient temperature for the verification model are assumed 20 W/m²K and 25°C, respectively. As can be seen, the obtained temperature in the eye along the pupillary axis is almost similar to the results from Shafahi and Vafai [33] as shown in Fig. 6. This favorable agreement between the two studies provides credence to the proposed model.

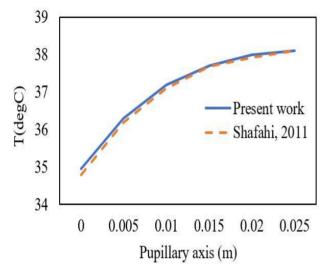


Fig. 6 Comparison of the temperature distribution inside the eye between present work and the work of Shafahi and Vafai.^[33]

3.2 Electric field intensity inside the eye

The EM radiation source moves on the port boundary of the model (Fig. 3) and scans the eye from the left side. The length

source is 5 mm. The EM source is in TE mode, operating at 900 and 1800 MHz frequencies with 1000 W power. The EM source takes 10 minutes to move across the port boundary. Fig. 7 shows the EM source positions at 0, 100, 200, 300, 400, 500, and 600 seconds. The electric fields propagate from the EM source through free space and incident on the eye where the tissues absorb it. Fig. 8 shows the electric field distribution in the eye at 0, 317, and 600 seconds for 900 and 1800 MHz frequencies. As can be seen the highest value of electric field intensity in the eye is found when the EM source has travelled 317 seconds and is now at a position very close to the eye. At this point of time, for both frequencies, the highest value of EM absorption in the eve is found in the cornea layer. Whereas, at 0 sec and 600 sec it is highest in the sclera layer. Cornea and sclera being the outermost layer of the eye and closer to the EM source gets more exposed. Hence, more absorption of the EM radiation is found in these layers. The EM distribution then diminishes as it goes deeper into the eye layers. Highest value of EM intensities at 0 sec (14.57 V/m) and 600 sec (15.40 V/m) are found for 900 MHz frequency. Whereas, for 317 sec (164.91 V/m) it is found for 1800 MHz frequency. Dielectric properties mentioned in Table 1 plays an important role in the EM absorption in the layers. The lower ε_r values of cornea and sclera when used in Eq. (1) causes easier penetration in the layers leading to higher values of electric field intensity. This absorbed energy in the layers then converts into the heat. Section 3.3 and 3.4 discusses the SAR and temperature distribution in the eye layers as a result of the absorption of EM field.

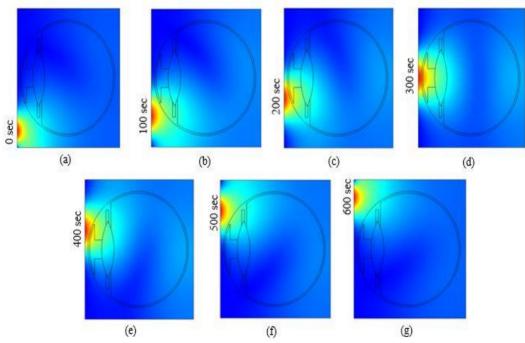


Fig. 7 Position of moving electromagnetic source from 0 to 600 seconds.

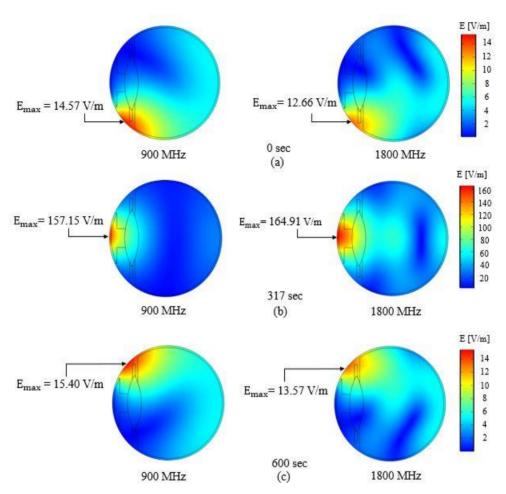


Fig. 8 Electric field distribution in the eye at (a) 0 sec, (b) 317 sec, and (c) 600 sec.

3.3 SAR distribution inside the eye

Figure 9 shows the SAR distribution in the eye layers as a result of the exposure from moving EM source at 900 and 1800 MHz frequencies. It is observed that similar to the electric field intensity (section 3.2), the highest value of SAR is found in the cornea layer of the eye at 317 sec for 1800 MHz frequency. However, at 0 sec and 600 sec it is found highest in the posterior chamber. The dielectric properties (σ , Table 1) and thermal properties (ρ , Table 2) plays an important role in calculating the SAR in the eye layers. The lower value of ρ in the posterior chamber than the sclera and higher value of σ in the posterior chamber than the sclera lead to higher value of SAR in the posterior chamber (Eq. 6). Highest value of SARs at 0 sec (0.17 W/kg) and 600 sec (0.19 W/kg) are found for 900 MHz frequency. Whereas for 317 sec (31.54 W/kg) it is found for 1800 MHz frequency. Considering the ICNIRP limits of 2 W/kg (general public exposure) and 10 W/kg (occupational exposure) for EM exposure, the SAR values obtained in the cornea at 317 sec exceeds the ICNIRP threshold values. This calculated SAR values are then used to calculate the temperature distribution inside the eye layers (section 3.4).

3.4 Temperature inside the eye

The temperature distribution inside the eye layers as a result of the exposure from EM radiation is calculated. A coupled model of electromagnetic wave propagation and bioheat transfer is solved numerically. The electric field intensity (Fig. 8) and SAR (Fig. 9) in the eye now converts into thermal energy leading to temperature increase. Fig. 10 shows the temperature distribution in the eye at three-time instants 0 sec, 317 sec, and 600 sec for 900 and 1800 MHz frequencies. Initial temperature in the eye has been set to 37°C. The electromagnetic source moves across the port boundary and irradiate the eye. The electromagnetic energy is then absorbed by the eye tissues. This absorbed energy in the tissues then transforms into heat increasing the overall temperature in the eye. At 0 sec, for both the frequencies, the maximum temperature in the eye is equal to the initial temperature. At 317 sec, the maximum temperature is found in the cornea layer of the eye for 1800 MHz frequency. Which is similar to electric field intensity and SAR distribution in the eye. However, at 600 sec, the maximum temperature in the eye is still in the cornea layer for 1800 MHz frequency. This does not follow the electric field intensity and the SAR distribution

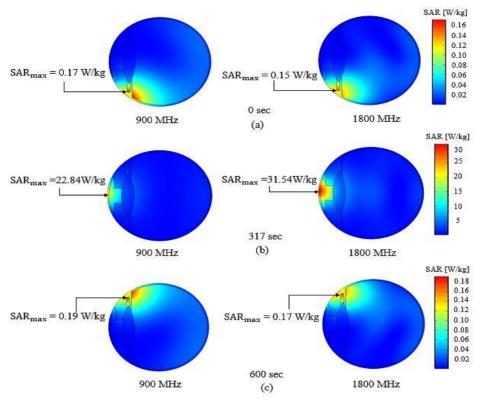


Fig. 9 SAR distribution in the eye at (a) 0 sec, (b) 317 sec, and (c) 600 sec.

cases. The maximum value of temperature at 0 sec is 37.0 °C, 3.5 Effect of the size of electromagnetic source at 317 sec is 37.72 °C, and at 600 sec is 37.44 °C. It is observed Effect of different sizes of EM source on the SAR and that the thermal properties from Table 2, highly influenced the temperature distribution in the eye has also been studied. Five temperature increase in the eye. However, this temperature sizes from 1 to 5mm are chosen for the EM source. increase is still very low to cause any harmful effect.

Comparison of SAR in the eye for different sizes of EM

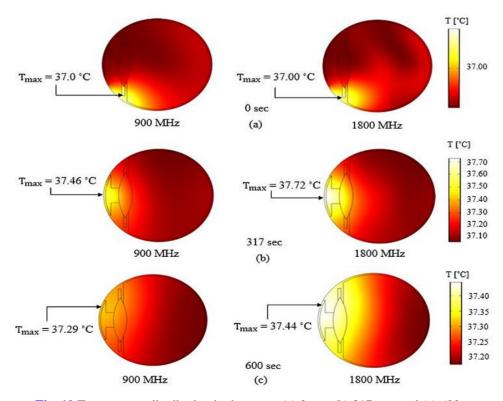


Fig. 10 Temperature distribution in the eye at (a) 0 sec, (b) 317 sec, and (c) 600 sec.

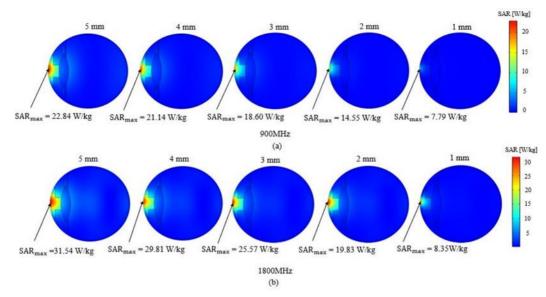


Fig. 11 Comparison of different sizes of electromagnetic source on the SAR in the eye at 317 sec position for (a) 900 MHz, and (b) 1800 MHz frequencies.

comparison has only been shown for the 317 sec position, as this is where the maximum absorption of EM energy in the eye is found. It can be seen from the results that the EM energy absorption in the eye is directly proportional to the size of the source. Larger the size of the EM source higher the SAR value in the eye. Smaller size EM source has low penetration and low absorption depth in the eye. It has also been observed that 1800 MHz frequency causes more absorption and penetration in the eye in comparison to 900 MHz frequency. This is because the dielectric properties of eye at 1800 MHz frequency are significantly higher than 900 MHz frequency (Table 1). The higher electrical conductivity and permittivity cause more absorption, Eq. (6). The temperature distribution

sources at both frequencies is shown in Fig. 11. The in the eye follows the SAR distribution, shown in Fig. 12. Just like SAR, higher value of temperature is found for the larger size of EM source. Also, 1800 MHz frequency showed more absorption and penetration depth of temperature in comparison to the 900 MHz. Higher value of SAR at 1800 MHz in comparison to 900 MHz leads to higher value of temperature at 1800 MHz according to Eq. (7) and (8). By comparing the SAR and temperature in the eye as a result of different sizes of EM source with the safety guidelines, it is concluded that the SAR values at all sizes exceeded the ICNIRP limit of 2 W/kg. However, the temperature increase in the eye has still found to be low to cause any serious adverse effect on the eye.[3,4]

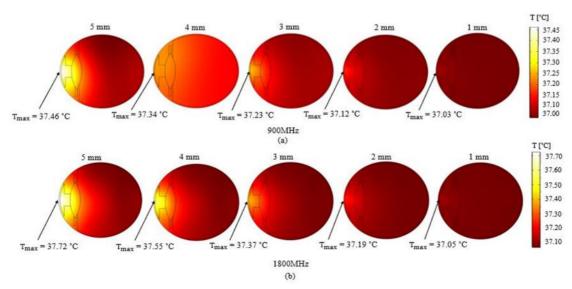


Fig. 12 Comparison of different sizes of EM source on the temperature in the eye at 317 sec position for (a) 900 MHz, and (b) 1800 MHz frequencies.

4. Conclusion

This study presents the absorption of EM radiation in a twodimensional human eve model as a result of the exposure from moving EM source propagating in TE mode at 900 and 1800 MHz frequencies with 1000 W power. The EM source takes total 10 minutes to move across the port and irradiate the eve from the left side. The results showed that the maximum value References of EM energy absorption occurs when the source is at 317 sec. This is the position when the distance between the EM source and the eye is smallest which leads to higher EM absorption in the eye. Maximum value of electric field intensity, SAR and temperature are found in the cornea layer of the eye at 317 sec position for 1800 MHz frequency. This is because cornea is the outermost layer of the eve, at 317 sec position of EM source, it gets more exposed in comparison to the other layers of the eye. Also, the dielectric properties of the eye at 1800 MHz frequency is higher than the 900 MHz frequency. This leads to more absorption of EM energy and SAR at 1800 MHz frequency which causes higher temperature. For 0 sec position, 10.1109/map.2003.1189664. the maximum value of electric field intensity is found in sclera layer (14.57 V/m at 900 MHz), maximum SAR is found in posterior chamber (0.17 W/kg at 900 MHz), and temperature is same for all layers (37.0 °C). For 600 sec, the maximum value of electric field intensity is found in sclera layer (15.40 V/m at 900 MHz), maximum value of SAR in posterior chamber (0.19 W/kg at 900 MHz), and maximum temperature in cornea layer (37.44°C at 1800 MHz). For 317 sec position, the maximum value of electric field intensity is found in cornea layer (164.91 V/m at 1800MHz), maximum value of SAR is also found in cornea layer (31.54 W/kg at 1800 MHz), and maximum temperature is also found in the cornea layer (37.72°C at 1800 MHz). Effect of different sizes of EM sources on the SAR and temperature distribution in the eye has also been studied. It was found that larger size of the EM source causes higher energy absorption in the eye. In all cases at 317 sec, the SAR value in the eye exceeded the limited exposure values. However, the temperature value in the eye is still below the threshold value to cause any adverse effect.

Acknowledgment

This study was supported by the Thammasat Postdoctoral Fellowship and Program Management Unit for Human Resources & Institutional Development, Research, and Innovation. **NXPO** (Grant Number B05F630092. B05F640205), National Research Council of Thailand (Grant Number N42A650197) and Thailand Science Research and Innovation Fundamental Fund (TU-FF 41/2566).

Conflict of Interest

There is no conflict of interest.

Supporting Information

Not applicable.

- [1] Guidelines for Limiting Exposure to Electromagnetic Fields (100 kHz to 300 GHz), International Commission on Non-Ionizing Radiation Protection (ICNIRP), Health Physics, 2020, 118, 483-524, doi: 10.1097/hp.000000000001210.
- [2] IEEE Standard for Safety Levels with Respect to Human Exposure to Electric, Magnetic, and Electromagnetic Fields, 0 Hz to 300 GHz, IEEE Std C95.1-2019 (Revision of IEEE Std C95.1-2005/ Incorporates IEEE Std C95.1-2019/Cor 1-2019), 2019, 1-312, doi: 10.1109/IEEESTD.2019.8859679.
- [3] J. C. Lin, Cataracts and cell-phone radiation, *IEEE Antennas* and Propagation Magazine, 2003, 45, 171-174, doi:
- [4] C. Buccella, V. De Santis, M. Feliziani, Prediction of temperature increase in human eyes due to RF sources, *IEEE* Transactions on Electromagnetic Compatibility, 2007, 49, 825-833, doi: 10.1109/temc.2007.909024.
- [5] T. Wessapan, P. Rattanadecho, Specific absorption rate and temperature increase in human eye subjected to electromagnetic fields at 900 MHz, Journal of Heat Transfer, 2012, 134, 1, doi: 10.1115/1.4006243.
- [6] A. W. Guy, J. C. Lin, P. O. Kramar, A. F. Emery, Effect of 2450-mhz radiation on the rabbit eye, IEEE Transactions on Microwave Theory and Techniques, 1975, 23, 492-498, doi: 10.1109/tmtt.1975.1128606.
- [7] P. Kramar, C. Harris, A. F. Emery, A. W. Guy, Acute microwave irradiation and cataract formation in rabbits and monkeys, Journal of Microwave Power, 1978, 13, 239-249, doi: 10.1080/16070658.1978.11689101.
- [8] Y. Kamimura, K.-i. Saito, T. Saiga, Y. Amemiya, Effect of 2.45GHz Microwave Irradiation on Monkey Eyes, *IEICE* Transactions on Communications, 1994, 77, 762-765.
- [9] O. P. Gandhi, G. Lazzi, C. M. Furse, Electromagnetic absorption in the human head and neck for mobile telephones at 835 and 1900 MHz, IEEE Transactions on Microwave Theory and Techniques, 1996, 44, 1884-1897, doi: 10.1109/22.539947.
- [10] O. Fujiwara, A. Kato, Approximation of Surface-SAR in a Realistic Head Model for Microwave Exposure Using External Magnetic Near-Field, IEICE Transactions on Communications, 1994, 77, 732-737.
- [11] J. Q. Lan, X. Liang, T. Hong, G. H. Du, On the effects of glasses on the SAR in human head resulting from wireless eyewear devices at phone call state, Progress in Biophysics and

Molecular Biology, 2018, 136. 29-36. 10.1016/j.pbiomolbio.2018.02.001.

- [12] K. Zarei, M. Lahonian, S. Aminian, S. Saedi, M. Ashjaee, Investigating the effect of wearing glasses on the human eyes' temperature distribution in different ambient conditions, Journal 2021. 99. 102971. of **Thermal** Biology, 10.1016/j.jtherbio.2021.102971.
- [13] M. S. Firoozan, S. Porkhial, A. S. Nejad, Effect of tissue and atmosphere's parameters on human eye temperature distribution, Journal of Thermal Biology, 2015, 47, 51-58, 10.1016/j.jtherbio.2014.11.001.
- [14] D. Bhargava, N. Leeprechanon, P. Rattanadecho, T. Wessapan, Specific absorption rate and temperature elevation in the human head due to overexposure to mobile phone radiation with different usage patterns, International Journal of Heat and Mass Transfer, 2019. 130. 1178-1188. 10.1016/j.ijheatmasstransfer.2018.11.031.
- [15] P. Bernardi, M. Cavagnaro, S. Pisa, E. Piuzzi, Specific absorption rate and temperature increases in the head of a cellular-phone user, IEEE Transactions on Microwave Theory and Techniques, 2000, 48, 1118-1126, doi: 10.1109/22.848494.
- [16] P. Bernardi, M. Cavagnaro, S. Pisa, E. Piuzzi, SAR distribution and temperature increase in an anatomical model of the human eye exposed to the field radiated by the user antenna in a wireless LAN, IEEE Transactions on Microwave Theory and Techniques, 1998, 46, 2074-2082, doi: 10.1109/22.739285.
- [17] P. Bernardi, M. Cavagnaro, S. Pisa, E. Piuzzi, Specific absorption rate and temperature elevation in a subject exposed in the far-field of radio-frequency sources operating in the 10-900-MHz range, IEEE Transactions on Biomedical Engineering, 2003, [28] J. Ma, X. Yang, Y. Sun, J. Yang, Thermal damage in three-**50**, 295-304, doi: 10.1109/tbme.2003.808809.
- [18] V. M. Flyckt, B. W. Raaymakers, H. Kroeze, J. W. Lagendijk, Calculation of SAR and temperature rise in a high-resolution vascularized model of the human eye and orbit when exposed to a dipole antenna at 900, 1500 and 1800 MHz, Physics in Medicine and Biology, 2007, 52, 2691-2701, doi: 10.1088/0031-9155/52/10/004.
- [19] A. Hirata, S.-I. Matsuyama, T. Shiozawa, Temperature rises in the human eye exposed to EM waves in the frequency range 0.6-6 GHz, IEEE Transactions on Electromagnetic Compatibility, [30] J. W. Hand, Modelling the interaction of electromagnetic 2000, **42**, 386-393, doi: 10.1109/15.902308.
- [20] A. Hirata, H. Watanabe, T. Shiozawa, SAR and temperature increase in the human eye induced by obliquely incident plane waves, IEEE Transactions on Electromagnetic Compatibility, 2002, 44, 592-594, doi: 10.1109/temc.2002.804778.
- [21] T. Wessapan, P. Rattanadecho, Aqueous Humor Natural Convection of the Human Eye induced by Electromagnetic Fields: [32] E. H. Amara, Numerical investigations on thermal effects of In the Supine Position, Journal of Medical and Bioengineering, 2014, **3**, 251-258, doi: 10.12720/jomb.3.4.251-258.

doi: [22] T. Wessapan, P. Rattanadecho, Temperature induced in human organs due to near-field and far-field electromagnetic exposure effects, International Journal of Heat and Mass Transfer. 2018. 119. 65-76. doi: 10.1016/j.ijheatmasstransfer.2017.11.088.

- doi: [23] T. Wessapan, S. Srisawatdhisukul, P. Rattanadecho, Specific absorption rate and temperature distributions in human head subjected to mobile phone radiation at different frequencies, International Journal of Heat and Mass Transfer, 2012, 55, 347-359, doi: 10.1016/j.ijheatmasstransfer.2011.09.027.
 - [24] D. Bhargava, P. Rattanadecho, T. Wessapan, The effect of metal objects on the SAR and temperature increase in the human head exposed to dipole antenna (numerical analysis), Case Studies in Thermal Engineering, 2020, 22, 100789, doi: 10.1016/j.csite.2020.100789.
 - [25] R. Inum, M. M. Rana, K. N. Shushama, M. A. Quader, EBG based microstrip patch antenna for brain tumor detection via scattering parameters in microwave imaging system, International Journal of Biomedical Imaging, 2018, 2018, 1-12, doi: 10.1155/2018/8241438.
 - [26] J. Ma, X. Yang, S. Liu, Y. Sun, J. Yang, Exact solution of thermal response in a three-dimensional living bio-tissue subjected to a scanning laser beam, *International Journal of Heat* 2018, 124, 1107-1116, and Mass Transfer, 10.1016/j.ijheatmasstransfer.2018.04.042.
 - [27] A. Kabiri, M. R. Talaee, Thermal field and tissue damage analysis of moving laser in cancer thermal therapy, Lasers in Medical Science, 2021, 36, 583-597, doi: 10.1007/s10103-020-03070-7.
 - dimensional vivo bio-tissues induced by moving heat sources in laser therapy, Scientific Reports, 2019, 9, 10987, doi: 10.1038/s41598-019-47435-7.
 - [29] P. Ninpetch, P. Kowitwarangkul, S. Mahathanabodee, P. Chalermkarnnon, P. Rattanadecho, Computational investigation of thermal behavior and molten metal flow with moving laser heat source for selective laser melting process, Case Studies in **Thermal** 100860, Engineering. 2021, 24. 10.1016/j.csite.2021.100860.
 - fields (10 MHz-10 GHz) with the human body: methods and applications, Institute of Physics and Engineering in Medicine, 2008, **53**, R243, doi: 10.1088/0031-9155/53/16/R01.
 - [31] J. A. Scott, A finite element model of heat transport in the human eye, Physics in Medicine and Biology, 1988, 33, 227-242, doi: 10.1088/0031-9155/33/2/003.
 - laser-ocular media interaction, International Journal of Heat and Mass Transfer, 1995, 38, 2479-2488, doi: 10.1016/0017-

9310(94)00353-W.

[33] M. Shafahi, K. Vafai, Human eye response to thermal disturbances, *Journal of Heat Transfer*, 2011, **133**, 011009, doi: 10.1115/1.4002360.

[34] S. Park, J. Jeong, Y. Lim, Temperature rise in the human head and brain for portable handsets at 900 and 1800, ICMMT 4th International Conference on, Proceedings Microwave and Millimeter Wave Technology, 2004, Beijing, China, 2004, 966-969, doi: 10.1109/ICMMT.2004.1411692.

[35] E. H. Ooi, E. Y. Ng, Simulation of aqueous humor hydrodynamics in human eye heat transfer, *Computers in Biology and Medicine*, 2008, **38**, 252-262, doi: 10.1016/j.compbiomed.2007.10.007.

Author Information



Dr. Deepshikha Bhargava received the Ph.D. degree in Engineering from Thammasat University, Thailand in 2021. She is currently working as a postdoctoral fellow in the same university. Her research interest includes computational electromagnetics, heat transfer in

biological tissues, antenna designing, and microwave imaging. Dr. Deepshikha has publications in some renowned journals. She also won a Gold medal at the "International British Innovation, Invention, Technology Expo (IBIX 2020), London, United Kingdom for designing an antenna for microwave imaging system for breast cancer detection.



Prof. Dr. Phadungsak Rattanadecho Received the Ph.D. degree in Mechanical engineering from Nagaoka University of Technology, in 2001. He is currently a professor at the department of Mechanical engineering in Thammasat University (rangsit

campus), Thailand. Dr. Phadungsak has produced more than 80 numerous published research papers in international academic journals. His work have been cited in international research database more than 900 times. His research interest includes multi-phase flow in porous media under electromagnetic energy and transport phenomena in highly complex systems by using statistical modelling.

Publisher's Note: Engineered Science Publisher remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.